

SICOM3009A Industrial Ethernet Switch

Hardware Installation Manual



KYLAND

Kyland Technology Co., LTD.

Publication Date: Oct. 2011

Version: V1.0

Customer Service Hotline: (+8610) 88796676

FAX: (+8610) 88796678

Website: <http://www.kyland.cn>

E-mail: support@kyland.biz

**SICOM3009A Industrial Ethernet Switch
Hardware Installation Manual**

Disclaimer: Kyland Technology Co., Ltd. tries to keep the content of this manual as accurate and as updated as possible. This document is not guaranteed to be error-free, and we reserve the right to amend it without notice to users.

**Copyright © 2011 KYLAND Technology CO., LTD.
All rights reserved.**

No part of this documentation may be excerpted, reproduced, translated, annotated or duplicated, in any form or by any means without the prior written permission of KYLAND Corporation.

Notice for Safety Operation

This product performs reliably as long as it is used according to the guidance. Artificial damage or destruction of the equipment should be avoided.

- Read this manual carefully and keep it for future reference;
- Do not place the equipment near water sources or damp areas;
- Do not place anything on power cable or put the cable in unreachable places;
- Do not tie or wrap the cable, which may cause a fire risk;
- Power connectors and other equipment connectors should be firmly interconnected and checked frequently;
- Do not repair the equipment by yourself, unless it is clearly specified in the manual;
- Please keep the equipment clean; if necessary, wipe the equipment with soft cotton cloth.

In the following cases, please immediately shut down your power supply and contact your Kyland representative:

- Water gets into the equipment;
- Equipment damage or shell damage;
- Equipment operation or performance has abnormally changed;
- The equipment emits odor, smoke or abnormal noise.

Contents

1	Packing List	4
2	Product Overview	4
3	Structure and Interface	5
3.1	Front Panel	5
3.2	Top Panel	10
4	Mounting.....	11
4.1	Dimension Drawing.....	11
4.2	Mounting Steps.....	12
5	Cable Connection	15
5.1	10/100Base-T(X) Ethernet Port.....	15
5.2	100Base-FX Ethernet Port.....	17
5.3	Console Interface.....	18
5.4	Power	19
5.5	Grounding.....	20
5.6	Relay Contact	22
6	LED Indicators	23
7	Reset Button.....	24
8	Management Access	25
8.1	Connected through Console Port.....	25
8.2	Connected through Ethernet Cable.....	27
8.3	Web Access.....	29
9	Product Configuration Information	29
10	Basic Features and Specifications	30

1 Packing List

SICOM3009A Industrial Ethernet Switch	1
CD	1
Screwdriver	1
18#AWG yellow-green line	1
Certificate of Quality (including Certificate of Compliance)	1

Note: After unpacking, please check the accessories and the appearance of the equipment. If anything is missing or damaged, please contact us.

2 Product Overview

SICOM3009A is a series of green low power consumption industrial Ethernet switch that can be applied extensively in wind power, distribution network automation, subway PIS、AFC, power SACDA, wastewater treatment, highway, metallurgy, hydroelectric power, photovoltaic power, railway CBTC, factory automation, intelligent transportation and many other industries.

SICOM3009A has a Mini USB Console port, and supports Web, Telnet and Console network management; supports VCT (Virtual Cable Test); supports one-key recovery.

SICOM3009A industrial Ethernet switch supports DIN-Rail and panel mounting. It provides six 10/100Base-T(X) ports and three Fast Ethernet fiber/RJ45 optional ports in the front panel.

3 Structure and Interface

3.1 Front Panel

- SICOM3009A-3S/M-6T

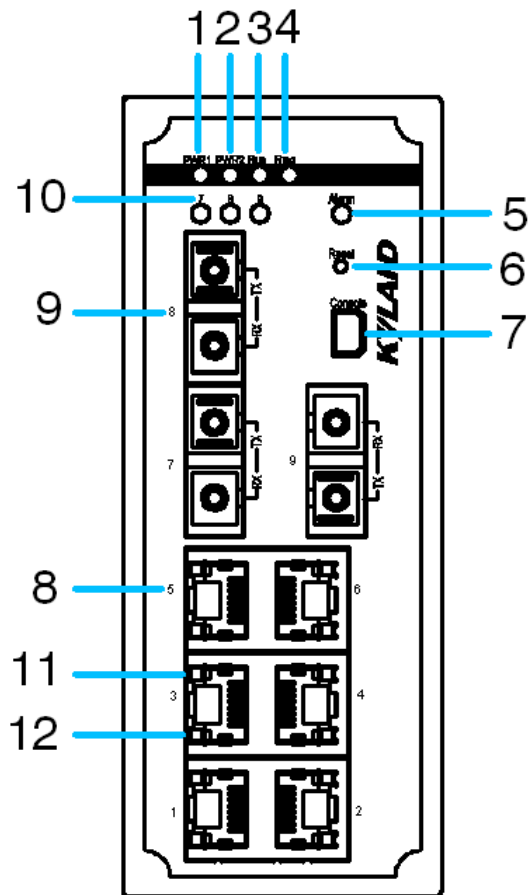


Figure 1 Front Panel 1

Table 1 SICOM3009A-3S/M-6T Front Panel

Number	Diagram Label	Description
1	PWR1	Power 1 LED
2	PWR2	Power 2 LED
3	Run	Running LED
4	Ring	Ring LED

5	Alarm	Alarm LED
6	Reset	Reset button
7	Console	Console interface
8	1~6	10/100Base-T(X) RJ45 port
9	7~9	100Base-FX port
10	7~9	100Base-FX port LED
11	--	RJ45 port Speed LED
12	--	RJ45 port Link/ACT LED

● SICOM3009A-2S/M-6T

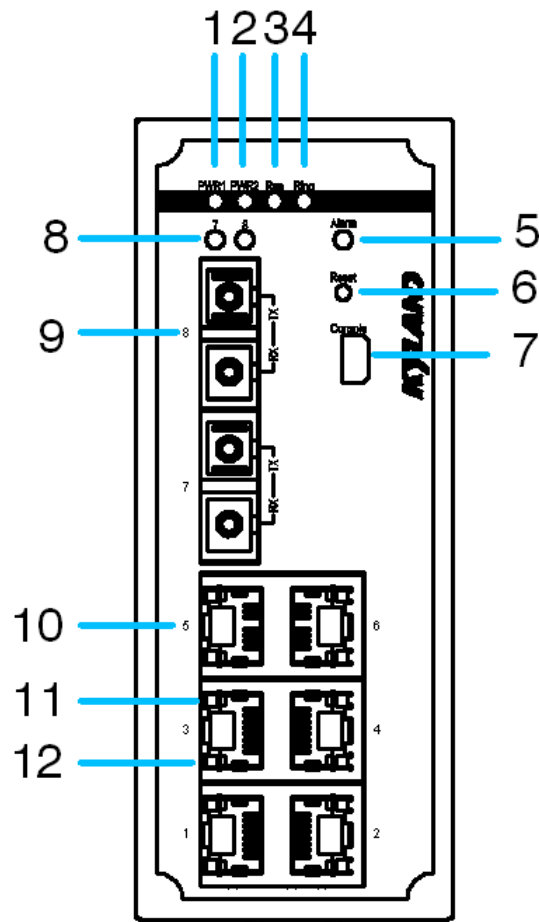


Figure 2 Front Panel 2

Table 2 SICOM3009A-2S/M-6T Front Panel

Number	Diagram Label	Description
1	PWR1	Power 1 LED
2	PWR2	Power 2 LED
3	Run	Running LED
4	Ring	Ring LED
5	Alarm	Alarm LED
6	Reset	Reset button
7	Console	Console interface
8	7, 8	100Base-FX port LED
9	7, 8	100Base-FX port
10	1~6	10/100Base-T(X) RJ45 port
11	--	RJ45 port Speed LED
12	--	RJ45 port Link/ACT LED

- SICOM3009A-1S/M-7T

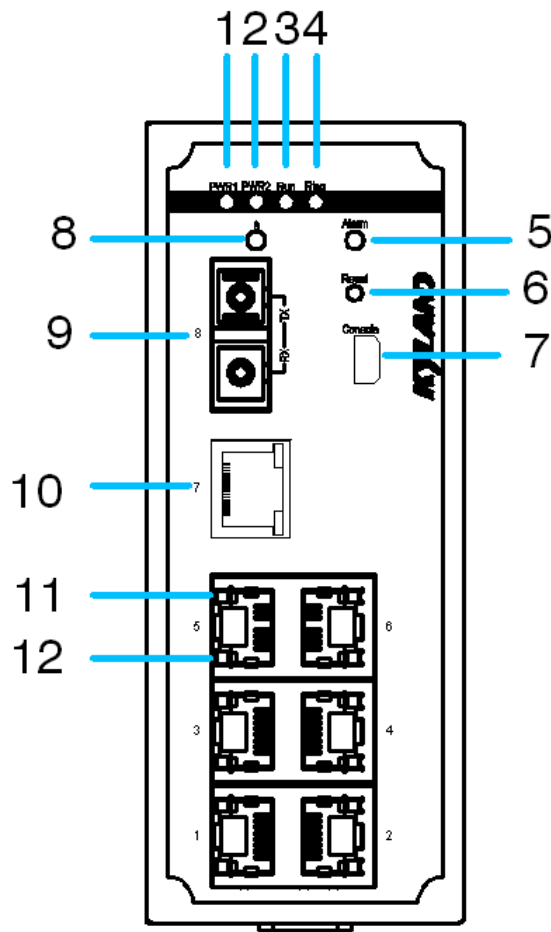


Figure 3 Front Panel 3

Table 3 SICOM3009A-1S/M-7T Front Panel

Number	Diagram Label	Description
1	PWR1	Power 1 LED
2	PWR2	Power 2 LED
3	Run	Running LED
4	Ring	Ring LED
5	Alarm	Alarm LED
6	Reset	Reset button
7	Console	Console interface
8	8	100Base-FX port LED

9	8	100Base-FX port
10	1~7	10/100Base-T(X) RJ45 port
11	--	RJ45 port Speed LED
12	--	RJ45 port Link/ACT LED

● SICOM3009A-8T

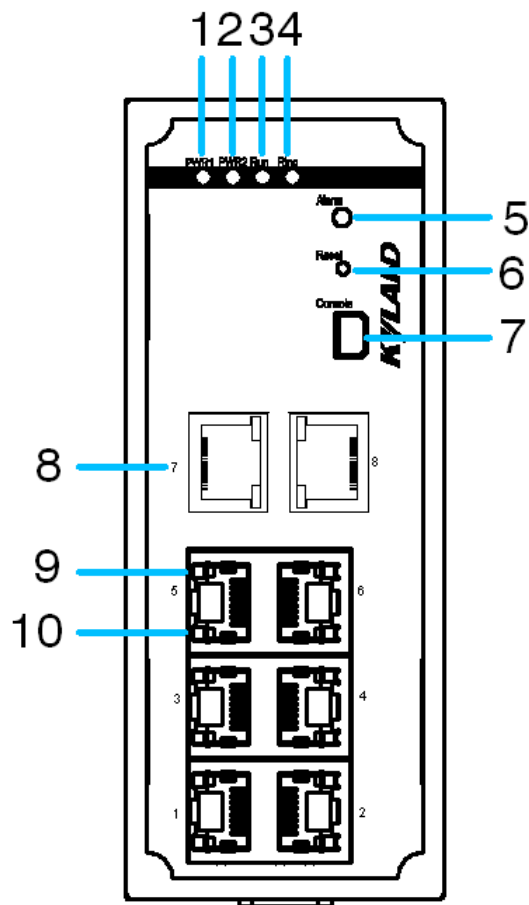


Figure 4 Front Panel 4

Table 4 SICOM3009A-8T Front Panel

Number	Diagram Label	Description
1	PWR1	Power 1 LED
2	PWR2	Power 2 LED

3	Run	Running LED
4	Ring	Ring LED
5	Alarm	Alarm LED
6	Reset	Reset button
7	Console	Console interface
8	1~8	10/100Base-T(X) RJ45 port
9	--	RJ45 port Speed LED
10	--	RJ45 port Link/ACT LED

3.2 Top Panel

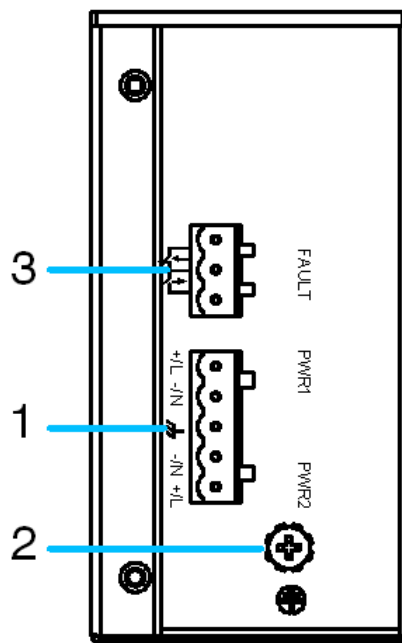


Figure 5 Top Panel

Table 5 SICOM3009A Top Panel

Number	Description
1	Power supply terminal block

2	Grounding Screw
3	Relay contact

4 Mounting

4.1 Dimension Drawing

- Dimension Drawing for DIN-Rail Mounting (Unit: mm)

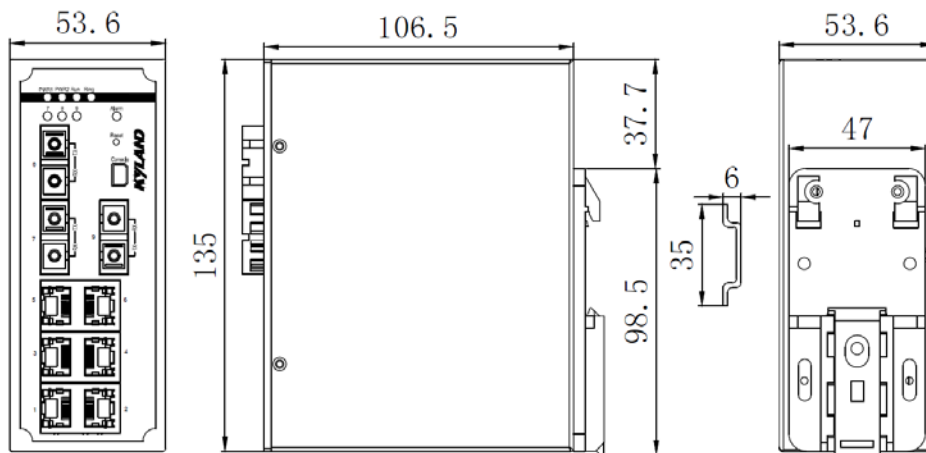


Figure 6 DIN-Rail Mounting Dimension

- Dimension Drawing for Panel Mounting (Unit: mm)

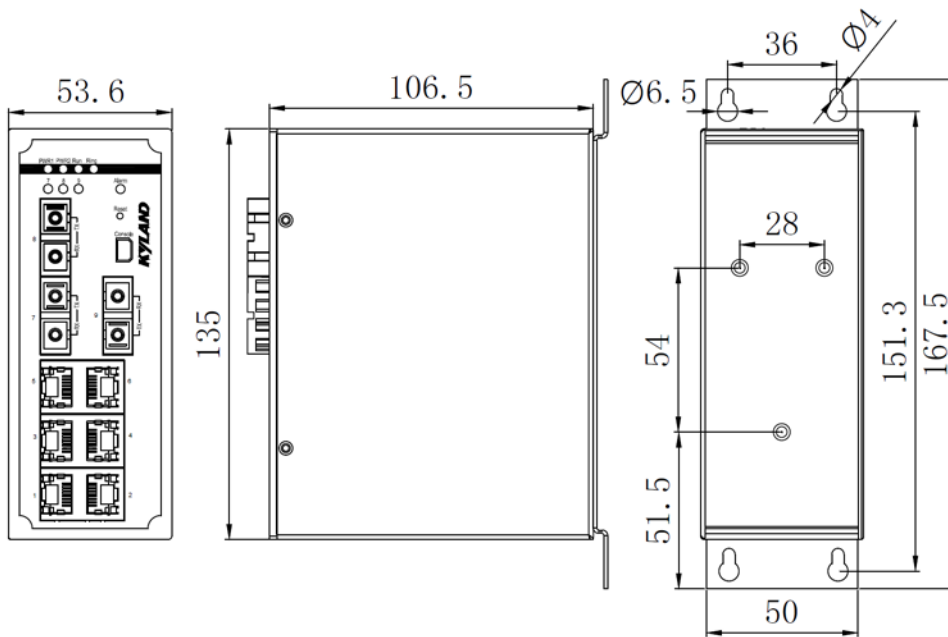


Figure 7 Panel Mounting Dimension

4.2 Mounting Steps

● SICOM3009A DIN-Rail Mounting

The specific steps are as follows:

Step 1: Select the mounting position for SICOM3009A and ensure that there is adequate space.

Step 2: Insert the top of the DIN-Rail into the slot of the DIN-Rail connecting seat in the rear panel of SICOM3009A as shown below; move the switch in the direction of arrow 2 to put the whole Din-Rail into the seat; check whether SICOM3009A is firmly mounted on the DIN-Rail, as shown below.

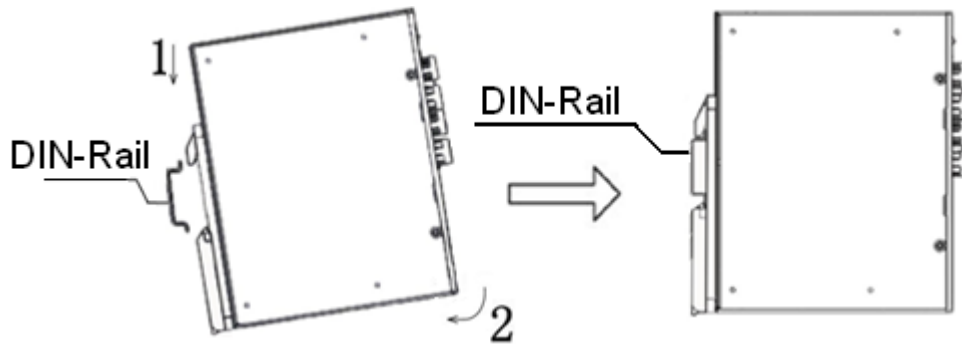


Figure 8 DIN-Rail Mounting

- Remove SICOM3009A from DIN-Rail

The specific steps are as follows:

Step 1: Insert the screwdriver into the hole at the bottom of spring locking plate; press the plate down to loosen the connection of DIN-Rail and switch, as shown in arrow 1.

Step 2: Pull the SICOM3009A up in the direction of arrow 2; meanwhile remove the switch from the DIN-Rail along the direction of arrow 3.

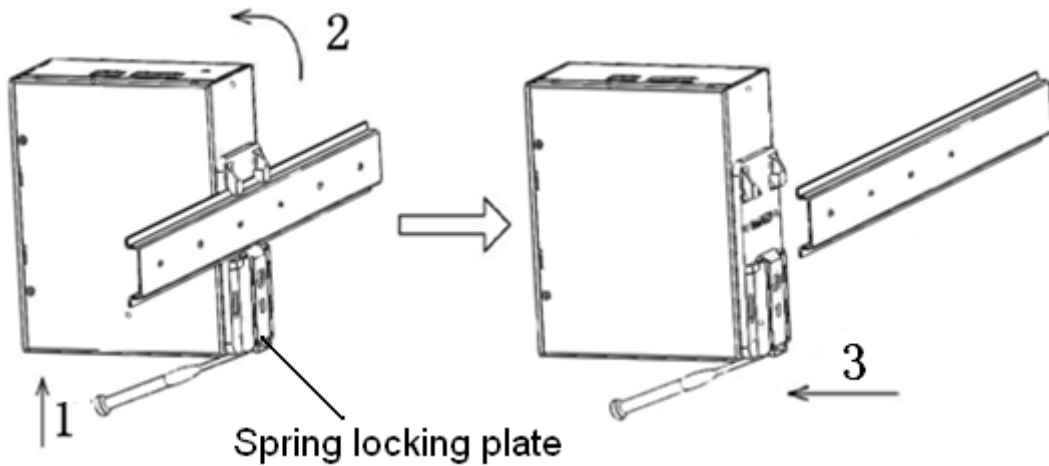


Figure 9 Dismounting

- SICOM3009A Panel Mounting

The specific steps are as follows:

Step 1: Select the mounting position for SICOM3009A on the wall or in

cabinet; ensure that there is adequate space for the switch.

Step 2: Drill 4 holes on the selected position according to the panel mounting dimension drawing; use a cross-screwdriver to screw 4 cross-slot screws (M3×10) into holes. Don't tighten the screws completely; leave about 5mm of space between.

Step 3: Aim 4 mounting holes on SICOM3009A mounting plate at 4 fixed screws; pass the screws through 4 holes with the diameter of 6.5mm ($\Phi 6.5$); then slide down SICOM3009A as seen below; finally screw 4 screws tightly. Now the SICOM3009A should be firmly fixed to the wall or cabinet.

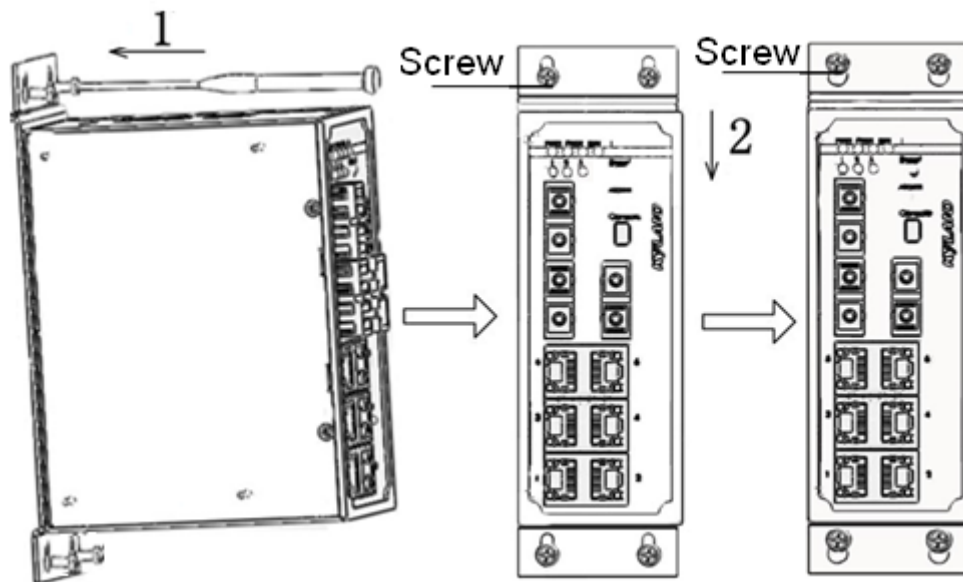


Figure 10 Panel Mounting

- Remove SICOM3009A from wall or cabinet

The specific steps are as follows:

Step 1: Use a screwdriver to loosen 4 screws; move the switch up to let screws into 4 holes with the diameter of 6.5mm ($\Phi 6.5$).

Step 2: Unscrew the screws from wall or cabinet; remove the switch from wall or cabinet.

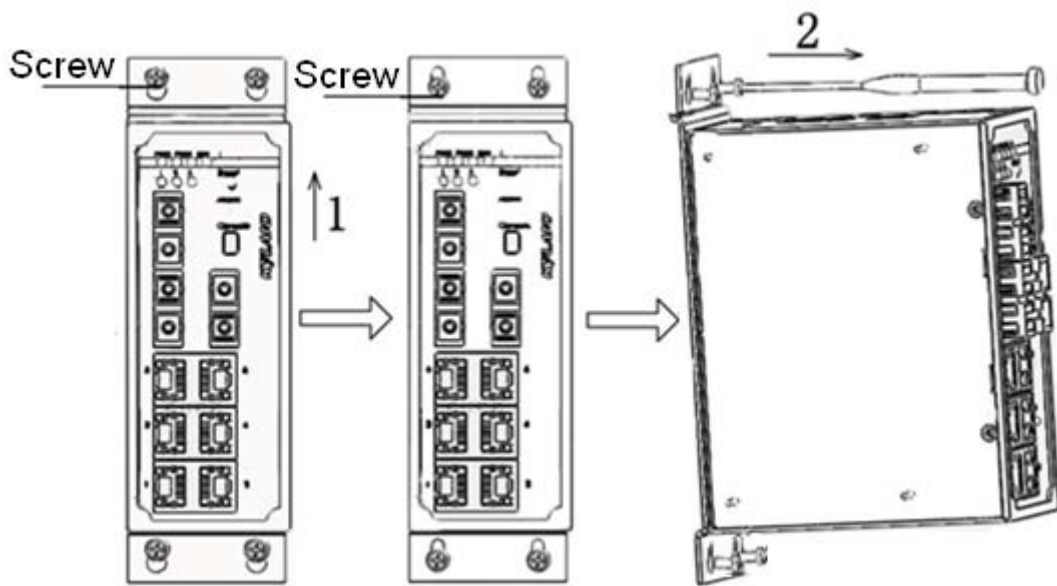


Figure 11 Dismounting

5 Cable Connection

5.1 10/100Base-T(X) Ethernet Port

10/100Base-T(X) Ethernet RJ45 port can be connected to terminal equipment and network devices with straight-through cables or crossover cables. RJ45 connectors must be equipped at both ends of cable.

- Pin definition of 10/100Base-T(X) RJ45 port

Pin number of 10/100Base-T(X) RJ45 port is shown in Figure 12




Figure 12 RJ45 Port

Pin definition of 10/100Base-T(X) RJ45 port is shown in Table 6

Table 6 Pin Definition of 10/100Base-T(X) RJ45 Port

Pin	MDI-X Signal Name	MDI Signal Name
1	Receive Data+ (RD+)	Transmit Data+ (TD+)
2	Receive Data- (RD-)	Transmit Data- (TD-)
3	Transmit Data+ (TD+)	Receive Data+ (RD+)
6	Transmit Data- (TD-)	Receive Data- (RD-)
4, 5, 7, 8	Unused	Unused

Note: "+" "-" means level polarity.

● Wiring Sequence

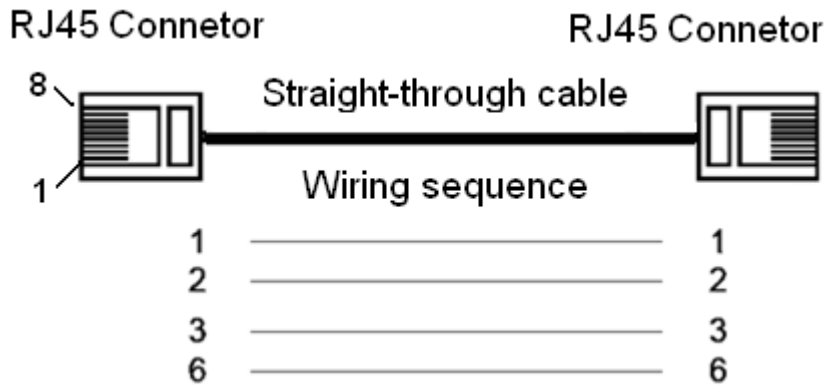


Figure 13 10/100M Straight-through Cable Wiring

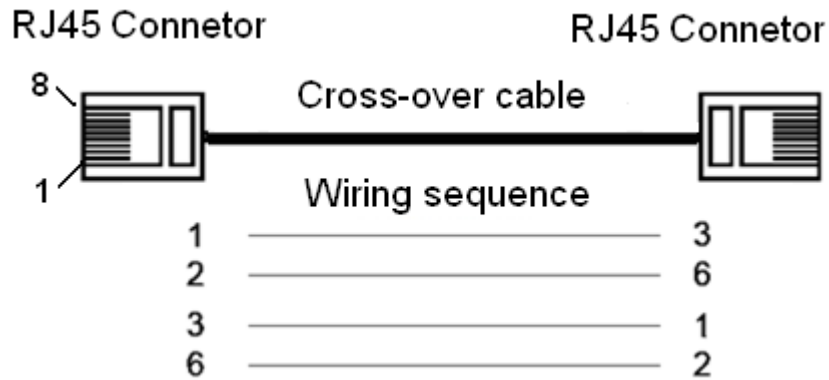


Figure 14 10/100M Cross-over Cable Wiring

Note: The correlation between the pin of RJ45 connector and the color of twisted pair is: 1-orange and white, 2-orange, 3-green and white, 4-blue, 5-blue and white, 6-green, 7-brown and white, 8-white.

5.2 100Base-FX Ethernet Port

100Base-FX Ethernet port is equipped with FC/SC/ST connector, and each port consists of TX (transmit) port and RX (receive) port, as shown in Figure 15.

100Base-FX port wiring is shown in Figure 15 (Take SC port as example; ST/FC wiring method is the same with SC). Connect the TX (transmit) port of switch A to the RX (receive) port of switch B, and the RX (receive) port of switch A to the TX (transmit) port of switch B in order to transmit data between switch A and switch B.

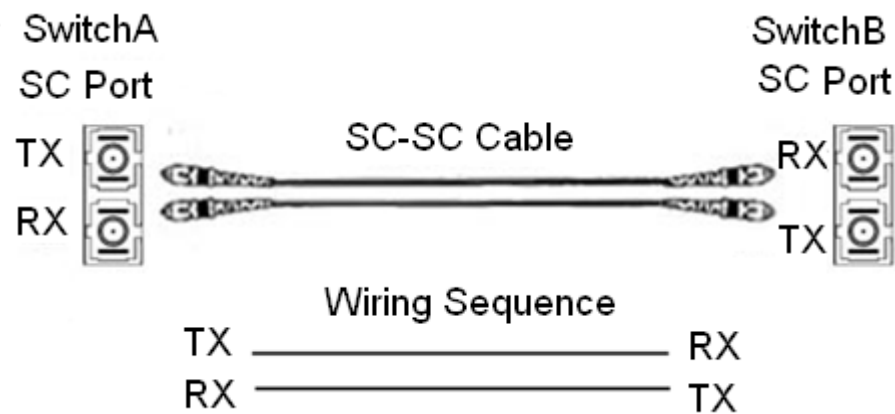


Figure 15 100Base-FX Port Wiring

Note: A laser is used to transmit signals in fiber cables. The laser meets the requirements of level 1 laser products. Routine operation is not harmful to your eyes, but do not look directly at the fiber port when the switch is powered on.

5.3 Console Interface

Install the driver for Mini USB onto your PC. The driver “Mini USB driver.exe” is in the software download folder, which is on the supplied CD. Connect the USB port on the PC to the Console interface on the switch with cable equipped with Mini USB connector and USB connector at both ends. Run Hyper Terminal software in WINDOWS operating system to connect to console software of the switch, which will allow you to configure, maintain and manage the switch.

- Mini USB connector

Mini USB connector pin number is shown in Figure 16.



Figure 16 Mini USB Connector

Mini USB connector pin definition is shown in Table 7.

Table 7 Mini USB Pin Definition

Mini USB Pin	Definition
1	VBUS
2	D-
3	D+
4	ID
5	GND

- USB connector

USB connector pin number is shown in Figure 17.

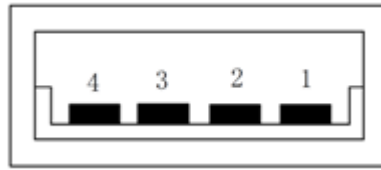


Figure 17 USB Connector

USB pin definition is shown in Table 8.

Table 8 USB Pin Definition

USB Pin	Definition
1	VBUS
2	D-
3	D+
4	GND

5.4 Power

According to the power input requirements, use a 5.08mm-spacing terminal block to connect power cable.

Note: The cross section area of power cable is required to be greater than 0.75mm² and less than 2.5mm². The grounding resistance requirement: <5Ω.

- 5 pin 5.08mm power terminal block

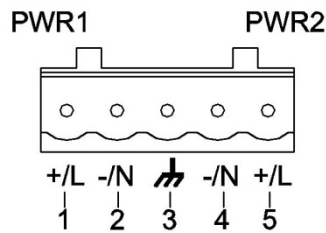


Figure 18 5-pin 5.08mm-spacing Plug-in Terminal Block

Table 9 5 Pin 5.08mm Power Terminal Block Contact Definition

Contact Number	DC Wiring Definition	AC Wiring Definition
1	PWR1: +	PWR1: L
2	PWR1: -	PWR1: N
3	Protection Ground	Protection Ground
4	PWR2: -	PWR2: N
5	PWR2: +	PWR2: L

- Wiring and mounting

Step 1: Take the power terminal block off the switch.

Step 2: Insert the power cable into the terminal block and connect the power cable.

Step 3: Put the terminal block back to the switch with the connected cable.

5.5 Grounding

- Chassis grounding and power terminal grounding

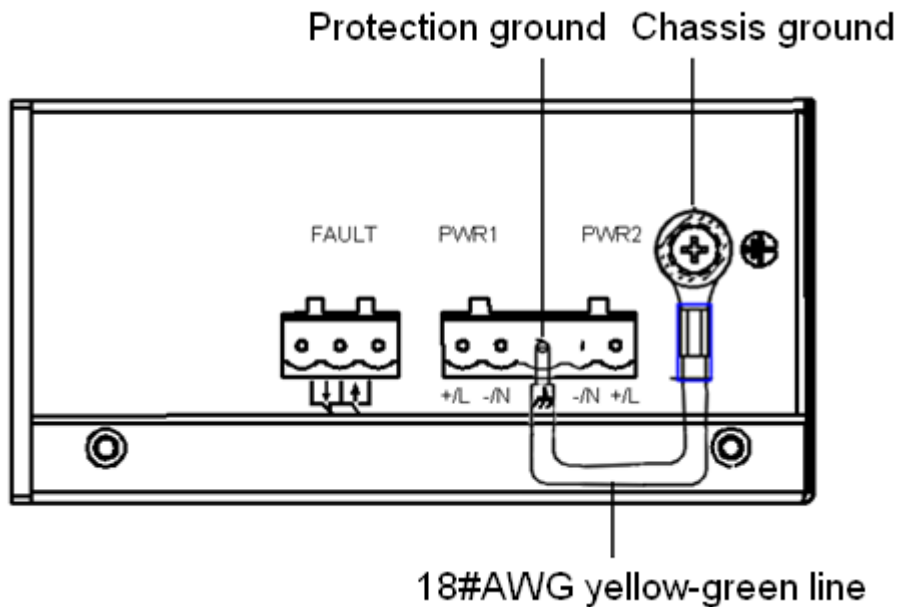


Figure 19 Chassis Grounding and Power Terminal Grounding

There is a grounding screw on the top panel of the SICOM3009A, which is for chassis ground. One end of the chassis grounding cable is connected with the grounding screw and the other end of the cable is reliably grounded. (The cross section area of chassis grounding cable should be more than 2.5mm^2 . The grounding resistance requirement: $<5\Omega$)

The grounding part in the 5.08mm power terminal block is called protection ground.

It is required to connect the chassis grounding part with the protection grounding part with supplied 18#AWG yellow-green line to allow the switch to operate safely and precisely.

The dimension drawing of 18#AWG yellow-green line is shown in Figure 20.

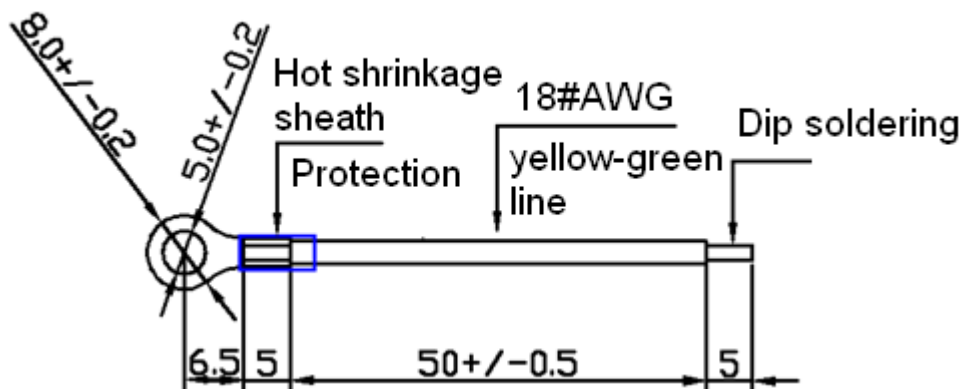


Figure 20 18#AWG Yellow-Green Line (Unit: mm)

Note: If SICOM3009A needs to perform a dielectric voltage withstand test, in order to avoid test failure, please disconnect the 18#AWG yellow-green line to disable surge protection circuit that leads to leakage electricity.

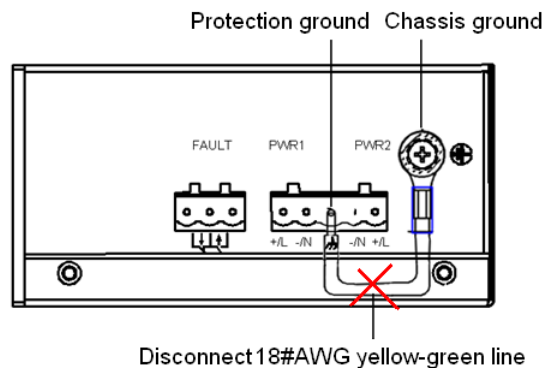


Figure 21 Disconnect 18#AWG Yellow-Green Line (Unit: mm)

5.6 Relay Contact

The relay contact is used for alarm output. When the switch works normally, the normally-open contact of the alarm relay is closed and the normally-closed contact is open; when the alarm occurs, the normally-open contact is open and the normally-closed contact is closed. The alarm is outputted through a 3-pin 5.08mm spacing terminal block as shown in Figure 22.




Figure 22 3-Pin 5.08mm-Spacing Plug-In Terminal Blocks

The electrical parameters of the relay:

Max Switch Voltage: 250VAC/220VDC;

Max Switch Current: 2A

Max Switch Power: 60W

Note: Pin 1 and pin 2 are normally-open contacts; pin 2 and pin 3 are normally-closed contacts. When the switch works normally, the pin 1 and 2 are closed, pin 2 and pin 3 are open; when the alarm occurs, the pin 1 and 2 are open; pin 2 and 3 are closed.

- **Wiring and mounting**

Step 1: Take the alarm terminal block off the switch.

Step 2: Insert the cable for alarm output into the alarm terminal block according to the requirements and connect the cable.

Step 3: Put the alarm terminal block back to the switch with the connected cable.

6 LED Indicators

Table 10 Front Panel LED

LED	State	Description
Running LED		
Run	ON	CPU is running abnormally or the switch is starting.
	Blinking (1HZ)	CPU is running normally
	OFF	CPU is not started up.
Alarm LED		
Alarm	ON	System alarm
	OFF	No system alarm.
Power LEDs		
PWR1	ON	Power 1 connects and operates normally.
	OFF	Power 1 disconnects or operates abnormally.
PWR2	ON	Power 2 connects and operates normally.

	OFF	Power 2 disconnects or operates abnormally.
Ring LED		
Ring	ON	Master (DT-Ring mode)/Root(DRP mode)
	Blinking	Slave (DT-Ring mode)/B-Root(DRP mode)
	OFF	No ring mode
10/100Base-T(X) RJ45 port LEDs		
Each RJ45 port has two indicators, a yellow LED and a green LED. The yellow LED indicates port rate, while the green LED indicates port connection state.		
Speed (Yellow)	ON	100M working state
	OFF	10M working state or no connection
Link/ACT (Green)	ON	Effective network connection in the port
	Blinking	Network activities in the port
	OFF	No effective network connection in the port
100Base-FX port LEDs		
Link/ACT	On	Effective network connection in the port
	Blinking	Network activities in the port
	Off	No effective network connection in the port

7 Reset Button

Reset button supports reboot and restoring default configuration.

Push the reset button and hold for one second then release to reboot the switch.

Hold the reset button down for five seconds then release to restore default configuration (including IP address) and reboot; the default IP address is **192.168.0.2**.

Note: Don't hold the reset button down for more than 5 second to avoid restoring default configuration.

8 Management Access

Access the switch by one of the following three ways.

8.1 Connected through Console Port

1. Install the driver for Mini USB onto your PC. The driver "Mini USB driver.exe" is in the software download folder, which is on the supplied CD.
2. Use the Console cable that is equipped with Mini USB connector at one end and USB connector at the other end to connect the Console interface on the switch with the USB port on PC.
3. On Windows desktop, click Start → All programs → Accessories → Communications → Hyper Terminal.

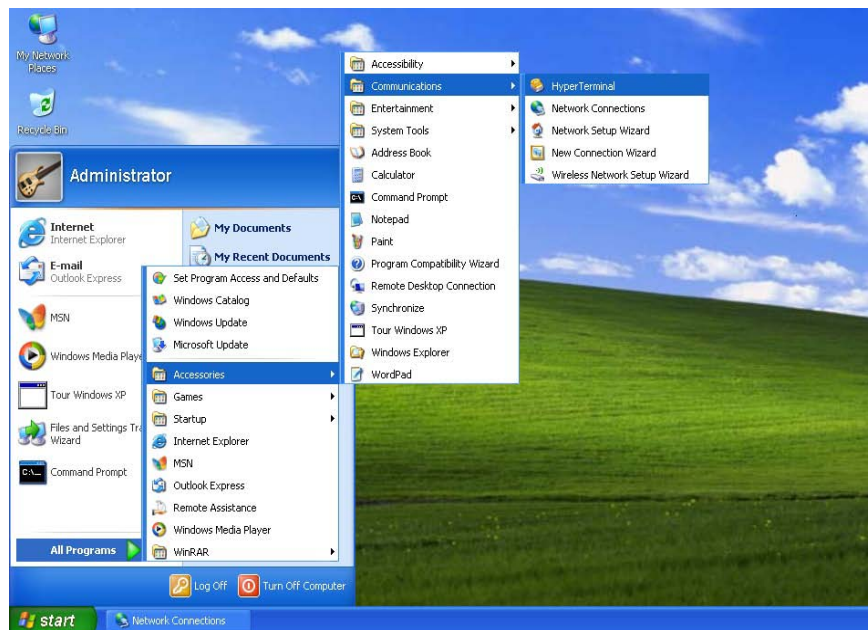


Figure 23 Hyper Terminal

4. Build a new connection named "aa"

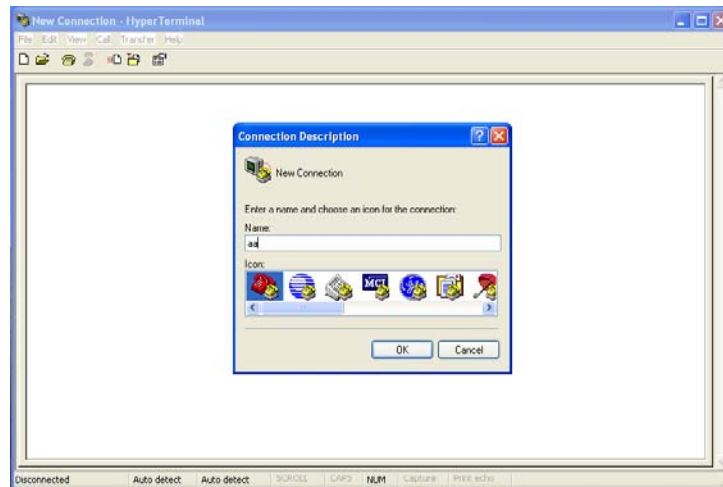


Figure 24 New Connection

5. Select COM port as the connection type.

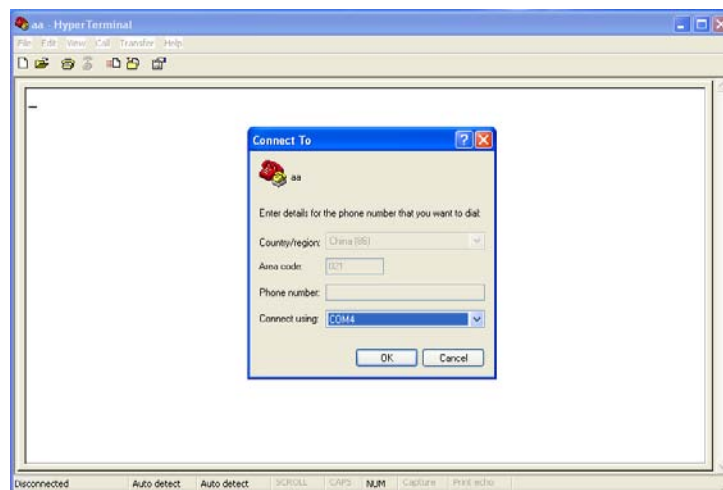


Figure 25 Choose Port

6. Set the parameters of COM port (Bits per second: 115200, Data bits: 8, Parity: None, Stop bits: 1, Flow control: None)

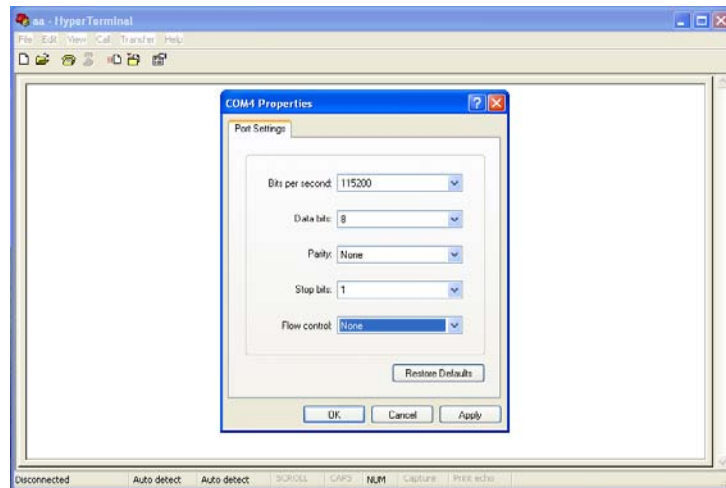


Figure 26 Set COM Parameters

- Click “OK” to enter the CLI interface, and type in a CLI command from Table 11.

Table 11 CLI Command

View	Command	Description
User View	SWITCH>enable	Enter management view
Management View	SWITCH#show interface	Show the IP address of current switch
Management View	SWITCH#show version	Show version of switch
Management View	SWITCH#reboot	Reboot
Management View	SWITCH#load default	Restore default configuration (except for IP address)
Management View	SWITCH#config terminal	Enter configuration view

8.2 Connected through Ethernet Cable

- Connect any RJ45 port of the switch with the Ethernet port of a personal computer with a RJ45 cable.
- Open Run window from the start menu, then input “telnet + ‘IP address’”.
The default IP address is **192.168.0.2**.

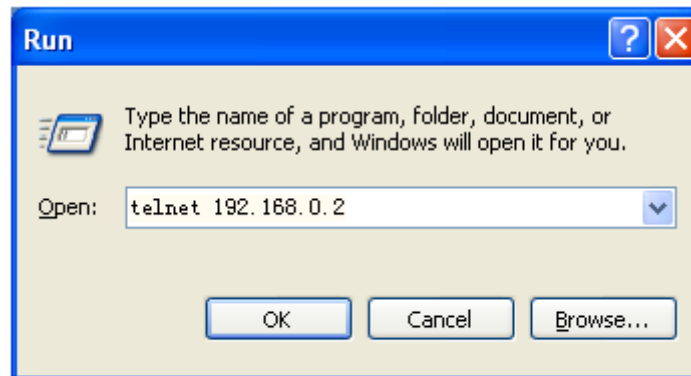


Figure 27 Enter Telnet

3. Click "OK" to enter the Telnet configuration interface. Type in a CLI command from Table 11.

8.3 Web Access

1. Connect the Ethernet port on the PC to any RJ45 port on the switch.
2. Input the IP address of the current switch in web browser, the default IP is **192.168.0.2**. The Web interface access screen will appear as shown below in Figure 28, login with default user name “**admin**” and password “**123**”.

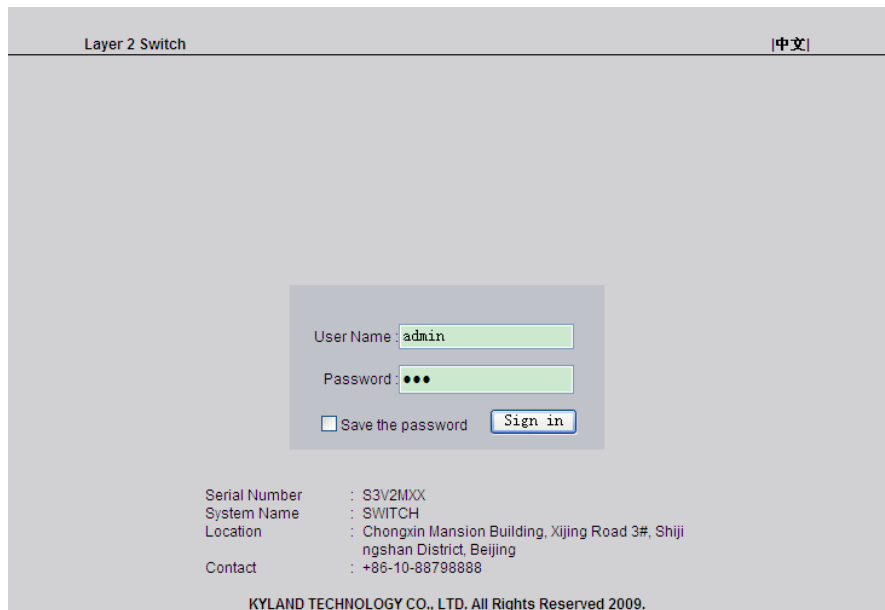


Figure 28 Web Interface Access Screen

Note: We recommend IE version 8.0 or greater.

9 Product Configuration Information

The specific configuration models of SICOM3009A are shown in Table 12.

Table 12 SICOM3009A Configuration

Model	Interface Description	Power
SICOM3009A-8T	8 10/100Base-T(X) RJ45 ports	12DC,
SICOM3009A-1S/M-7T	1 100Base-FX, SM/MM ports, FC/SC/ST	24AC/DCW

	connector; 7 10/100Base-T(X) RJ45 ports	dual redundant power inputs
SICOM3009A-2S/M-6T	2 100Base-FX,SM/MM ports, FC/SC/ST connector; 6 10/100Base-T(X) RJ45 ports	
SICOM3009A-3S/M-6T	3 100Base-FX,SM/MM ports, FC/SC/ST connector; 6 10/100Base-T(X) RJ45 ports	

Table 13 SICOM3009A Optional Accessories

Model	Description
DT-BGAZ-02	Panel mounting kit
DT-FCZ-RJ45-01	RJ45 dustproof shield
DT-XL-Mini USB-USB-2m	USB console cable, Mini USB to USB, 2m

10 Basic Features and Specifications

- Power Requirements

Power input: 12DC (9~18VDC),

24AC/DCW (18~72VDC, 18~50VAC)

Power terminal: 5-pin 5.08mm-spacing plug-in terminal block

Power consumption: SICOM3009A-8T: 5.1W (MAX)

SICOM3009A-1S/M-7T: 5.6W (MAX)

SICOM3009A-2S/M-6T: 6.1W (MAX)

SICOM3009A-3S/M-6T: 6.6W (MAX)

- Physical Characteristics

Housing: Metal, fanless

Installation: DIN-Rail or panel mounting

Dimensions (W×H×D): 53.6mm×135mm×106.5mm

Weight: 0.76Kg

- Environment Limits

Operating Temperature: -40°C~+85°C

Storage Temperature: -40°C~+85°C

Ambient Relative Humidity: 5%~95% (non-condensing)

- MTBF

350877h

- Warranty

5 years

For more information about KYLAND products, please visit our website:

<http://www.kyland.cn/>